

This Page Is Inserted by IFW Operations
and is not a part of the Official Record

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

IMAGES ARE BEST AVAILABLE COPY.

**As rescanning documents *will not* correct images,
please do not report the images to the
Image Problem Mailbox.**

PATENT COOPERATION TREATY

From the INTERNATIONAL BUREAU

PCT

NOTIFICATION OF ELECTION

(PCT Rule 61.2)

To:

Commissioner
US Department of Commerce
United States Patent and Trademark
Office, PCT
2011 South Clark Place Room
CP2/5C24
Arlington, VA 22202
ETATS-UNIS D'AMERIQUE

in its capacity as elected Office

Date of mailing (day/month/year)

20 February 2002 (20.02.02)

International application No.

PCT/HU01/00028

Applicant's or agent's file reference

TENSIOPILL

International filing date (day/month/year)

07 March 2001 (07.03.01)

Priority date (day/month/year)

09 March 2000 (09.03.00)

Applicant

ILLYÉS, Miklós

1. The designated Office is hereby notified of its election made:



in the demand filed with the International Preliminary Examining Authority on:

15 October 2001 (15.10.01)



in a notice effecting later election filed with the International Bureau on:

2. The election ☐ was



was not

made before the expiration of 19 months from the priority date or, where Rule 32 applies, within the time limit under Rule 32.2(b).

RECEIVED
JUN 20 2002
TECHNOLOGY CENTER R3700

The International Bureau of WIPO
34, chemin des Colombettes
1211 Geneva 20, Switzerland

Facsimile No.: (41-22) 740.14.35

Authorized officer

Maria KIRCHNER

Telephone No.: (41-22) 338.83.38

PATENT COOPERATION TREATY

PCT

INTERNATIONAL SEARCH REPORT

(PCT Article 18 and Rules 43 and 44)

Applicant's or agent's file reference TENSIOPILL	FOR FURTHER ACTION <small>see Notification of Transmittal of International Search Report (Form PCT/ISA/220) as well as, where applicable, item 5 below.</small>	
International application No. PCT/HU 01/ 00028	International filing date (day/month/year) 07/03/2001	(Earliest) Priority Date (day/month/year) 09/03/2000
Applicant ILLY S, Mikl s		

This International Search Report has been prepared by this International Searching Authority and is transmitted to the applicant according to Article 18. A copy is being transmitted to the International Bureau.

This International Search Report consists of a total of 3 sheets.
☒ It is also accompanied by a copy of each prior art document cited in this report.

1. Basis of the report

a. With regard to the **language**, the international search was carried out on the basis of the international application in the language in which it was filed, unless otherwise indicated under this item.

☐ the international search was carried out on the basis of a translation of the international application furnished to this Authority (Rule 23.1(b)).

b. With regard to any **nucleotide and/or amino acid sequence** disclosed in the international application, the international search was carried out on the basis of the sequence listing :

☐ contained in the international application in written form.

☐ filed together with the international application in computer readable form.

☐ furnished subsequently to this Authority in written form.

☐ furnished subsequently to this Authority in computer readable form.

☐ the statement that the subsequently furnished written sequence listing does not go beyond the disclosure in the international application as filed has been furnished.

☐ the statement that the information recorded in computer readable form is identical to the written sequence listing has been furnished

2. ☐ **Certain claims were found unsearchable** (See Box I).

3. ☐ **Unity of invention is lacking** (see Box II).

4. With regard to the **title**,

☒ the text is approved as submitted by the applicant.

☐ the text has been established by this Authority to read as follows:

5. With regard to the **abstract**,

☒ the text is approved as submitted by the applicant.

☐ the text has been established, according to Rule 38.2(b), by this Authority as it appears in Box III. The applicant may, within one month from the date of mailing of this international search report, submit comments to this Authority.

6. The figure of the **drawings** to be published with the abstract is Figure No.

☒ as suggested by the applicant.

☐ because the applicant failed to suggest a figure.

☐ because this figure better characterizes the invention.

1, 2
☐ None of the figures.

(19) World Intellectual Property Organization
International Bureau



(43) International Publication Date
13 September 2001 (13.09.2001)


PCT

(10) International Publication Number
WO 01/66061 A1


- (51) International Patent Classification⁷: A61J 7/00
- (21) International Application Number: PCT/HU01/00028
- (22) International Filing Date: 7 March 2001 (07.03.2001)
- (25) Filing Language: English
- (26) Publication Language: English
- (30) Priority Data:
P 0001103 9 March 2000 (09.03.2000) HU
P 0100911 28 February 2001 (28.02.2001) HU
- (71) Applicant and
(72) Inventor: ILLYÉS, Miklós [HU/HU]; Kétújfalu u. 163,
H-1182 Budapest (HU).
- (74) Agent: POLGÁR, Iván; DeveloPat Patent Agency, P.O.
Box 21, H-1400 Budapest (HU).
- (81) Designated States (*national*): AE, AG, AL, AM, AT, AU, AZ, BA, BB, BG, BR, BY, BZ, CA, CH, CN, CO, CR, CU, CZ, DE, DK, DM, DZ, EE, ES, FI, GB, GD, GE, GH, GM, HR, HU, ID, IL, IN, IS, JP, KE, KG, KP, KR, KZ, LC, LK, LR, LS, LT, LU, LV, MA, MD, MG, MK, MN, MW, MX, MZ, NO, NZ, PL, PT, RO, RU, SD, SE, SG, SI, SK, SL, TJ, TM, TR, TT, TZ, UA, UG, US, UZ, VN, YU, ZA, ZW.
- (84) Designated States (*regional*): ARIPO patent (GH, GM, KE, LS, MW, MZ, SD, SL, SZ, TZ, UG, ZW), Eurasian patent (AM, AZ, BY, KG, KZ, MD, RU, TJ, TM), European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE, TR), OAPI patent (BF, BJ, CF, CG, CI, CM, GA, GN, GW, ML, MR, NE, SN, TD, TG).
- Declaration under Rule 4.17:**
— *of inventorship (Rule 4.17(iv)) for US only*
- Published:**
— *with international search report*

[Continued on next page]

(54) Title: APPARATUS FOR DOSAGE OF MEDICAMENTS

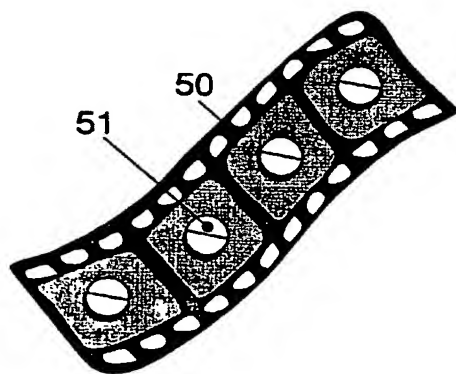

(57) Abstract: The subject matter of the invention is an apparatus to dose medicaments and control taking in the medicaments, which apparatus consists of a storage unit (5) to store tablets or capsules, a dosing unit and a counter (7). The characteristic feature of the apparatus according to invention is that the medicaments (like tablets or capsules) (51) are packed in a medicament tape (50) and stored in the storage unit (5) and cylinders (1) furthering said medicament tape (50) are attached to the storage unit (5) and the said cylinders are mechanically coupled with a manual driving unit (4).

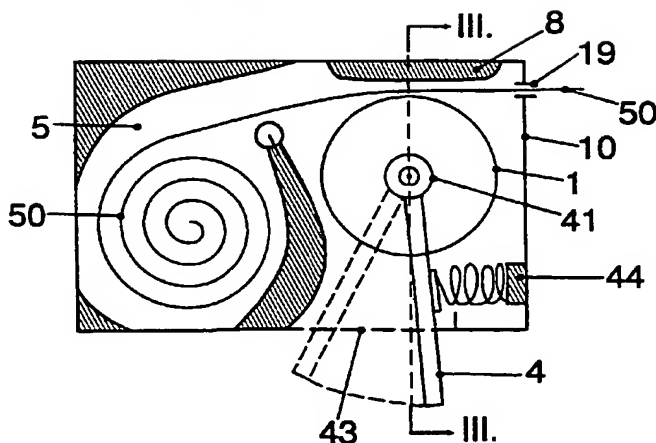

WO 01/66061 A1



— with amended claims and statement

For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.

APPARATUS FOR DOSAGE OF MEDICAMENTS

The field of the invention

An apparatus to dose medicaments and to control taking them, which apparatus consists of a tablet or capsule storage unit, a dosage unit and a counting unit, as
5 well.

Description of the state of art

Apparatuses serving for dosage medicament tablets or similarly shaped products, like table dosing apparatuses of saccharin or lemon salt are well-known for a long time past. These dosage apparatuses are based on the principle, that a cassette is
10 arranged under a container which holds tablets in bulk mass, and the cassette is movable against a spring force. The cassette is open both on the upper and lower sides. A pill or tablet falls from the container into the cassette. The cassette is moved into the other sector of dosing apparatus, where the bottom of cassette has an opening, the pill or tablet falls out. A treatment of a patient with prescribed
15 medicaments requires an apparatus of higher quality and accuracy. Such apparatus is described in the patent application PCT/US96/0387, which comprises an event counter. The characteristic feature of this apparatus is that a display unit can be cyclically operated in an on and an off status. The counting is coupled with the electric switching on and off the apparatus. The patient carries the apparatus with
20 himself and it counts and records all the events occurring during the treatment. The apparatus has a disadvantage that the dosage of medicament and the counting are not interlocked.

No one of the known apparatuses affords a solution to control, how the patient cooperates with his physician and whether he takes the prescribed medicament in at
25 the prescribed time. If he deviates from the prescription, how long e. g. the deviation time is. Such data are necessary both in the viewpoint of the treatment and for recognition of efficiency of the applied medicament, as well.

It is furthermore necessary, that such data were available in great quantity, in a reliably recorded and well applicable for processing form. Actually no apparatus is known, which is reliable, easy to use and widespread applicable in the physician's practice and medical attendance.

5

Description of the invention

The destination of this invention is to develop an apparatus for dosage of medicaments, which can be manufactured simply, with low expenses, and its application enables the physician to get knowledge about co-operation of the treated patient, observance of the prescribed cure, by this way the real efficiency
10 of the applied medicament on one hand. On the other hand, the physician's opinion about the medicaments can become more grounded. Another aim of this invention is, to interlock the counting with the effectively dosed medicament units in the apparatus according to this invention.

The invention is based on the recognition, that the tape-shaped package of tablets,
15 pills or capsules in a common blister pack makes it possible to dose the said tablets, pills, or capsules only one by one at any time with simultaneous counting of them, using a simple mechanism and a minimum of electronic equipment. Not only the quantity of dosed medicament units can be recorded by means of an appropriate electronic equipment, but the time of dosage, as well. If the co-
20 operative behaviour (compliance) of patient is associated with the taking the medicament in the prescribed time, the data collected by the apparatus according to invention, deliver information necessary both for medical treatment and for real evaluation of efficiency of the medicament in question.

Another recognition underlying the invention is, that tablets, pills or capsules
25 packed in a tape-shaped common blister pack can be administered simply, hygienically and accurately in a counting and dosing apparatus, which comprises a storage unit containing the medicament in a wound tape, and a dosing one consisting of a tape furthering unit, a shifting one, and, if necessary, a cutting one.

We recognised, that the stepwise movement of tape can be performed by the length of one medicament unit at each time even in the simplest embodiment without cutting unit.

5 A cutting unit becomes automatically wound up at the movement of the shifting unit and it is released at the end of movement by a prescribed length and cuts the tape in another advanced embodiment of the apparatus.

It belongs to the recognitions, that the separate furthering and cutting makes possible a relatively slow furthering followed by an instantaneous cutting. The furthering of the tape and cutting of a medicament unit are, however not
10 simultaneous by this way but one after the other, nevertheless they are bound inseparably together by means of a simple automatic mechanism. It is required that if a furthering has begun, it should not be ceased, but it should be performed anyway on the whole designed length. The movements on partial distances can cause an erroneous positioning of the tape and the cutting can destruct the tablets.
15 We recognised furthermore, that the above mentioned partial movements caused by a partially actuated shifting unit can be eliminated, if the shifting unit rests in the reached position and a following movement can only complete the previous one.

All the embodiments carried out on the base of the above mentioned recognitions
20 can comply with the aim set above, but they have different reliability. It should be considered in any case, whether a simpler, consequently cheaper apparatus or a more exigent, consequently more expensive one should be chosen.

A supplement of the inventive recognitions is, that several advantages can be obtained if an electronic counter, which registers the patient's co-operative
25 behaviour (compliance), is attached to the system as an exchangeable unit. The physician's evaluation becomes easier and the counter becomes reusable even in the case, when the dosing unit used only once and then disposed.

The inventive solution is an apparatus for dosage of medicaments and control of taking in them, the apparatus based on the above mentioned recognitions consists
30 of a storage unit, which stores the capsules or tablets to be dosed, a dosing unit and a counter. The characteristic feature of the solution according to invention is

that furthering cylinders are mounted onto the container which stores the medicament units (either tablets or capsules, packed into a tape shaped blister pack), and the said cylinders are mechanically coupled with a hand operated driver unit.

- 5 The apparatus according to invention can be advantageously characterised by that it is equipped with a cutting unit, which serves to disjoint one by one the segments of the tape containing medicament units.

Another advantageous feature of the apparatus is that the counter comprises a mechanic signal transmitter, an electronic sensor, an internal clock and a memory unit.

10 A further advantageous feature of the apparatus according to invention is that the driver unit is coupled with the signal transmitter, which transmits a signal to the sensor at each dosing of medicament units. The coupling can be a direct or an indirect one, it can be established e.g. either by the shifting unit and/or by the axle.

- 15 The apparatus according to invention can be advantageously characterised by that the driving unit is mechanically coupled with a cutting unit. and actuates it.

A following advantageous feature of the apparatus according to invention is that the driving unit is coupled with the cylinders through a stepping mechanism equipped with a position stabiliser and an inhibitor unit.

- 20 The embodiment with inhibitor unit can be advantageously characterised that the stepping unit is equipped with lifting units, which lift the stepping one to an ineffective position and releasing ones which eliminate the lifting.

A further advantageous embodiment of the apparatus according to invention can be characterised that one of the cylinders is equipped with a unit winding up the cutting unit, namely with a cutting gearwheel, and with a unit releasing it. i. e. initiating the cut namely a cylinder lifting unit.

- 25 Finally, the apparatus according to invention can be advantageously characterised that the counter is exchangeable by its shape and dimensions, and it is mounted onto apparatus using a known in itself solution and can be simply inserted, taken out or changed.
- 30

The invention is shown by means of the attached drawings without any limitation of the extent of protection claimed and the possible embodiments of the invention to the shown embodiments.

5 The figures:

Figure 1: View of the tape shaped blister pack of medicament.

Figure 2: Simplified side view with section of the apparatus according to invention

Figure 3: Simplified section of the apparatus shown in the Figure 2 according the
III-III plane

10 Figure 4: Simplified side view with section of another advantageous embodiment
of the apparatus according to invention

Figure 5: Simplified section of the apparatus shown in the Figure 4 according to V-
V plane

15 Figure 6: Simplified side view of the embodiment of the apparatus according to
invention with cutting unit

Figure 7: Simplified section by horizontal plane of the apparatus shown in Figure 6

Figure 8: Section of the stepping unit of the embodiment shown in Figure 6

Figure 9: Coupling of the stepping and inhibitor unit in the embodiment shown in
Figure 6

20 Figure 10: Detail drawings in section of the fastening and releasing units of the
inhibitor unit.

Figure 11: Detail drawings in section of the fastening and releasing units of the
inhibitor unit with other arrangement.

25 Figure 12: Detail drawing showing the guide of stepping unit and the inhibitor unit
in section

Figure 13: Detail drawing showing the lifting unit of the arresting one in section

30 According to the invention the tablets 51 which can be any medicament units i. e.
tablets, pills or capsules are packed into a blister pack tape 50 arranged
equidistantly in one row along the length of tape (Figure 1). The tape can be made
of any known in itself foil or synthetic film. The medicament tape 50 consists of
two layers and the tablets are arranged between the layers as mentioned above.

One of borders or both borders of the medicament tape 50 can be provided with a guiding row of holes similarly to film-strips or computer printer paper for a feeding mechanism with sprocket wheel, if necessary. It is sufficient even the antiskid treatment of the borders to further the tape. The medicament tape is

5 provided advantageously with perforation or weakened at the section in the half distance between the tablets. The apparatus according to the invention is mounted into housing 10. A part of this housing is the storage unit 5. (Figure 2). The medicament tape 50 is housed in it in wound up state. In the other part of housing 10 is mounted a cylinder 1 fastened on an axle 2. The axle 2 is mounted in

10 bearings 21 shaped in the housing 10 and it can be rotated. An arm shaped driving handle is coupled with the axle through a ratchet motion 41 (Figure 3). The driving handle 4 projects out of the housing 10 through an opening 43. The dimensions of the opening enables the driving handle to turn by an angle that the curved surface of cylinder 1 moves the medicament tape further by the length of

15 one tablet.

The driving handle 4 is coupled with a basic spring 44, its other end is fastened to the housing 10. A guiding element 8 is arranged above the cylinder 1 which can be substituted by a row of rolls. The free end of the medicament tape 50 stored in the storage unit 5 goes between the cylinder 1 and the guiding element 8 to the outlet

20 opening 19 in the wall of the housing 10. The curved surface of the cylinder 1 can be even or provided with pins for a medicament tape 50 with guiding holes or the cylinder 1 can be substituted with a combination of cylinder with sprocket-wheels. The cylinder-1 has a groove 17 which lets the tablets go through. A signal

25 transmitter 72 is fastened onto the axle 2, too. The signal transmitter 72 is a disc with cams on its circumference. The cams are arranged evenly, their number is equal to that of tablets 51 being in the part of medicament tape 50 which covers the perimeter of cylinder 1. A sensor 71 is fastened against the signal transmitter 72, which issues an electric output signal under pressure. The counter 7 includes furthermore an evaluating unit 74, an internal clock connected to it, and a memory

30 unit 75 connected to the evaluating unit. All the electronic units are known in themselves commercial products, and they are assembled by ordinary way, as

well. A further simple embodiment of the apparatus according to invention deviates from the above described one, that an annular gear is shaped on the perimeter of the ratchet motion 41 and the driving handle 4 is a gear rack 42 mounted vertically in relation to the axle 2 (Figures 4 and 5). The driving handle projects out of the housing 10 through the opening 43 and it is mounted so that it can be moved only "vertically", i. e. perpendicularly to the plain of the opening 43. The gear rack 42 is engaged with the annular gear of the ratchet motion 41. The movement of the driving handle is limited by stops to a span, which corresponds to a pivot of cylinder 1 to further a tablet 51. The movement of driving handle 4 is performed against force of at least one basic spring 44 which is released when the driving handle 4 projects out of the housing 10 and is wound up when the said handle is pushed in. Advantageously the apparatus can be equipped with a manual cutting unit (not shown for simplicity). The latter is mounted onto the housing 10 next to the outlet opening 19. It can be e. g. a blade guided by rail or turning around a pivot and actuated by hand in both cases. The cutting unit is positioned so that it cuts in the middle of distance between two tablets. A more advanced version of the apparatus according to invention includes an automatic cutting unit 9. The driving handle 4 is coupled to the cylinders 1 through a stepping unit 3 and at least one of said cylinders 1 is coupled to the cutting unit 9. The subassembly, which furthers the medicament tape 50 consists of three cylinders 1 (see Figure 6) the axles thereof are arranged like lateral edges of a prism of triangular basis. All the cylinders are provided with groove 17 in the middle of their curved surfaces. The locations of cylinders are different. A driven cylinder 12 is installed advantageously next to the storage unit. The driven cylinder 12 is coupled with the pressing cylinder 11 on one hand and with the cutting cylinder 13 on the other hand. Gear wheels 14 are mounted on the axles of each cylinder in one plain, they establish the coupling between them. (see Figure 7) There are cutting gear wheels 15 mounted on the both ends of the cutting cylinder 13 nearer to the cylinder as the coupling gearwheel 14. Their diameters are greater than those of gear wheels 14 and they can be arranged because a gap exists wider than said wheel 15 between the driven cylinder 12 and its coupling gear wheel 14. A stepping unit 3

is coupled to the gear wheel 14 of the driven cylinder 12 (see Figure 8). It is a rod of square profile, coupled to the gear wheel 14 of the driven cylinder 12 through a gear rack 31. The stepping unit 3 is guided through coupled ribs and grooves in a guiding element 36 arranged on both longitudinal sides of the stepping unit 3 (see Figure 12). The stepping unit 3 is coupled to the opposite wall of apparatus by a stepping spring 38, where a mechanic sensing button 71 of an electronic counter 7 is fastened. A breaking edge 32 is shaped on the opposite (lower) side of the stepping unit to the gear rack 31. The breaking edge 32 is provided with triangular teeth and it is coupled to an inhibitor unit 6 (see Figure 9). The inhibitor unit 6 includes a ratchet-closing device 61, the tongue 65 thereof is stressed to the triangular teeth of the braking edge 32. There are lifting shoulders 62 on both sides of the inhibitor unit 6 (see Figure 13), their height together with the lifting arms 33 is greater than the penetration depth of the tongue 65 i. e. the depth of teeth on the braking edge 32. The inhibitor unit 6 is equipped with fixing clips 63 (see Figures 10, 11) which are mounted onto pins and they are turnable under spring pressure around the pins and they engage into cavities 67 on both frontal ends of the inhibitor unit 6. The stepping unit is equipped with at least two clip releasing units 37 which contact with the advantageously extended ends of the fixing clips 63 on the opposite side of the said pin in the basic position of the stepping unit 3. A cutting unit 9 including two toothed racks 93 which hold a knife 91 on its both sides and they are pressed by a cutting spring 94 towards the storage unit 5 (see Figure 7). The axle 2 of the cutting cylinder 13 is supported by bearings with springs and a roll 16 is fastened on its end. A cylinder lifter 35 extends from the stepping unit 3 to the said roll 16. The surface of the wall of storage unit 5 is shaped as guiding surface 8 under the cylinders 1 on the side facing to the knife 91 and it is provided with a cutting groove 81 parallel to the axles 2.

The counter 7 is advantageously fitted into a compartment corresponding to its shape and dimensions, with an inner opening to the signal transmitter and being accessible from the outer side of the housing 10. The counter 7 is fastened into the said compartment by clamp joint or any other releasable fastening known in itself.

The apparatus functions and it can be used by the following way. First the physician determines the cure and the medicament. He loads then the medicament in the form of medicament tape 50 into the storage unit 5, and leads the free end of the tape between the cylinders 1 or between a cylinder and a guiding surface 8. He closes the housing 10 with a seal. If a simple embodiment shown in Figures 2 to 4 is used, the patient either moves the driving handle as the opening 43 lets it to move (see Figures 2, 3) or pushes it inwards until it stops (see Figures 4, 5). He turns the cylinder 1 by an angle, that it moves the medicament tape forward by the length of a tablet sector 51. He tears off the part of the medicament tape 50 containing a tablet 51 run out at the perforation, or he cuts it off, if the apparatus is equipped with a cutting instrument. The signal transmitter 72 issues a signal to the sensor 72 at the dispensing of each tablet, and an electronic signal enters the evaluating unit 74. from the said sensor. The evaluating unit calls the actual time from internal clock 73 and records both the event of dispensing and the incidental time in the memory unit 75. The I/O connection of the counter 7 enables to call the data for processing. This embodiment can properly function only if it is properly used. The driving handle should be moved along the whole allowed path and the moved segment should be cut off at each time.

In another advanced embodiment the stepping unit 3 is moved forward by pushing down the driving handle 4. The gear rack 31 is engaged with the gear wheel 14 of the driven cylinder 12. The driven cylinder 12 moves the medicament tape 50 forward exactly by a length of a section containing one tablet 51 at one whole movement of the stepping unit 3, as result of properly determined dimensions. If a pushing cylinder 11 is applied above the driven cylinder 12, a pair of gear wheels ensure the synchronised rotation of cylinders 1. A medicament tape 50 with leading row of holes is moved forward by means of pins on the cylinders 1 or sprocket wheels mounted on the sides of said cylinders 1. The tablets 51 pass through groove or grooves in the one or more cylinders 1 applied, this way they are not damaged by passing the cylinders 1. The free end of medicament tape 50 is lead between the driven cylinder 12 and the cutting cylinder 13 and then it reaches the guiding surface 8. At the start the medicament tape should be positioned so

that the beginning of the section containing the first tablet 51 be exactly at the cutting groove 81. The medicament tape moves forward by a section of medicament tape 50 containing one tablet 51, and the line between two tablets 51 steps to the cutting groove 81 at each actuation of the driving handle 4 after this
5 positioning. The cutting unit 9 functions as follows: While the driven cylinder 12 moves, it turns the cutting cylinder 13 through gear wheels 14. The cutting cylinder moves the toothed racks 93, at the same time the complete cutting unit 9 in the direction opposite with the movement of stepping unit compressing the cutting springs 94 and accumulating energy in them. Before the stepping unit
10 reaches its final position, the cylinder lifting arm 35 fastened on it reaches the roll 16 on the end of axle 2 of the cutting cylinder 13 (Figure 7), and detaches the cutting gear wheel 15 from the gear rack 93. The energy of cutting springs 94 pushes forward the cutting unit 9 so that the knife 91 lashes into the cutting groove 81 and cuts off a tablet 51 from the medicament tape 50. The tablet 51 falls
15 into a dispensing nest. The stepping unit 3 reaches its final position and issues a signal to the counter 7 by pushing the sensor 71 (Figure 8). When the driving handle is released, the stepping spring 38 pushes back the stepping unit 3 and the driving handle 4 into their basic positions. The cylinder lifting arm 35 moves backwards and it does not lift the cutting cylinder any more, the cutting gear wheel
20 15 and gear rack 93 are re-engaged. When the driving handle 4 is pushed down again, the cutting unit 9 becomes wound up again. This apparatus works reliably, if the user operates it accurately, and he pushes the driving handle 4 always up to stop i. e. until the cutting unit 9 is released and lashes into the cutting groove 81. If he does not take care of it he pushes down the driving handle 4 only partially, then
25 releases it and tries to push once more, the medicament tape 50 gets into wrong position and the cutting edge 92 may touch a tablet 51.

The partial movement of the driving handle 4 is inhibited in a further advantageous embodiment. The inhibitor unit 6 functions as follows: The backward movement of the stepping unit 3 caused by the stepping spring 38 is
30 inhibited by the catch device 61 of the inhibitor unit 6, the tongue 65 thereof catches the teeth of the breaking edge 32 on the lower part of stepping unit 3. If

the patient does not push the driving handle 4 and the stepping unit 3 down up to the stop, the later is fixed in the position of partial movement (see Figure 9). This state remains up to the moment, when the lifting arms 33 of the stepping unit 3 reach the lifting shoulders 62 on the sides of inhibitor unit 6 (see Figure 13). At the moment of contact the braking edge 32 and the catch device 61 are detached. The inhibitor unit 6 is pushed down against the inhibitor springs 66 and the fixing clips 63 enter into cavities 67 on its sides, as the inhibitor unit 6 reaches their height (Figures 10 and 11). These fixing clips 63 fasten the inhibitor unit 6 independently from the lifting arms 33. Being detached from the inhibitor unit 6 the stepping unit 3 returns into its basic position under force of stepping spring 38. The clip releasing units 37 engage with the fixation releasing elements 64 and the fixing clips step out of the cavities 67. The inhibitor unit 6 re-engages with the stepping unit 3. Consequently, there is a cyclic procedure in the actuation of the apparatus. When the stepping unit 3 is moved partially forward, the inhibitor unit 6 prevents its movement backwards until the stepping unit reaches its desired final position. In this moment the effect of the inhibitor unit 6 terminates, the stepping unit 3 returns to its basic position, and the inhibitor unit 7 returns into basic position at the same time, as well, and re-enters its effect. The counter 7 works by the same way as described above.

At the end of treatment the counter 7 is taken out of the housing 10, connected to the physician's computer and its data content is evaluated. Having deleted the data content, the counter 7 can be re-inserted into a housing 10 reloaded with a new dose of medicament or, if the apparatus is designed for single usage, the counter 7 can be used for a new apparatus.

The apparatus according to invention is a new combination built up of mechanic and electronic elements known in themselves. It fulfils important medical and health care requirements: it informs the attending physician, whether the prescribed cure was performed according to prescriptions, and the planned medical effect was reached at the actual patient at one hand. On the other hand, it provides reliable data for the statistical evaluation of the efficiency of medicaments eliminating all the doubts originating from the deficit of knowledge

of patients. All the energy consuming elements of the apparatus are mechanical structures, which are driven by hand of patient. The energy requirement of the electronic part is very low, so it can be reliably used for long time. The applied package of the medicament is also advantageous because the whole quantity of
5 medicament necessary for the cure is loaded in a hygienic package by the physician into the dosing apparatus.

CLAIMS

1. An apparatus for dosing medicaments serving to control the taking in prescribed medicaments, which apparatus consists of a storage unit, which stores the tablets or capsules to be dosed, a dosing unit and a counting one,
5 **characterised by that medicament units (51) (either capsules or tablets) packed in a medicament tape (50) are stored in a storage unit (5) and cylinders (1) furthering said medicament tape (50) are attached to the storage unit (5) and the said cylinders are mechanically coupled with a manual driving unit (4).**
2. The apparatus according to Claim 1, characterised by that the apparatus is
10 equipped with a cutting unit which serves to cut off a segment of the medicament tape (50).
3. The apparatus according to the Claims 1 or 2, characterised by that a counter (7) is attached to the apparatus, which comprises a mechanic signal transmitter (72), an electronic sensor (71), an electronic evaluating unit (74) electrically
15 connected to said sensor, an internal clock (73) and a memory unit (75).
4. The apparatus according to Claim 3, characterised by that the driving unit (4) is coupled with the signal transmitter (72) issuing a signal to the sensor (71) at dosing of each tablet.
5. The apparatus according to any one of the Claims 1 to 4 characterised by that
20 the driving unit (4) is coupled with a cutting unit (9) in a manner to control the latter, which corresponds to the above mentioned cutting unit.
6. The apparatus according to any one of the Claims 1 to 5 characterised by that the driving unit (4) is coupled with the cylinders (1) through a stepping unit (3) equipped with an inhibitor unit (6) stabilising the position.
- 25 7. The apparatus according to Claim 6 characterised by that the stepping unit (3) is equipped with lifting arms (33) which lift the inhibitor unit into an ineffective position and with releasing arms (37) which eliminate the lifting.
8. The apparatus according to any one of the Claims 1 to 7 characterised by that at
30 least one of the cylinders (1) is equipped with an unit winding up the cutting unit (9), namely with a cutting gear wheel (15) and the stepping unit (3) is

equipped with a unit eliminating the winding up of the cutting unit (9), namely a cylinder lifter (35).

9. The apparatus according to any one of the Claims 3 to 8 characterised by that the counter (7) is built up and fastened in the apparatus as an exchangeable unit.

AMENDED CLAIMS

[received by the International Bureau on 24 July 2001 (24.07.01);
original claim 1 replaced by new claim 1; original claims 3-9 renumbered as claims 3-7 (1 page)]

1. An apparatus for dosing medicaments serving to control the taking in prescribed medicaments, which apparatus consists of a storage unit, a dosing unit and a counting one, wherein the medicament units (either capsules or tablets) to be dosed, packed in a medicament tape are stored in the storage unit and cylinders furthering said medicament tape are attached to the storage unit, and the said cylinders are mechanically coupled with a manual driving unit, **characterised by that**, a counter (7) is attached to the apparatus, which comprises a mechanic signal transmitter (72), an electronic sensor (71), an electronic evaluating unit (74) electrically connected to said sensor, an internal clock (73) and a memory unit (75), and the driving unit (4) is coupled with the signal transmitter (72) issuing a signal to the sensor (71) at dosing of each tablet.
2. The apparatus according to Claim 1, characterised by that the apparatus is equipped with a cutting unit (9), which serves to cut off a segment of the medicament tape (50).
3. The apparatus according to the Claims 2, characterised by that the driving unit (4) is coupled with the cutting unit (9) in a manner to control the latter.
4. The apparatus according to Claim 2 or 3, characterised by that the driving unit (4) is coupled with the cylinders (1) through a stepping unit (3) equipped with an inhibitor unit (6) stabilising the position.
5. The apparatus according to the Claims 4 characterised by that the stepping unit (3) is equipped with lifting arms (33) which lift the inhibitor unit (6) into an ineffective position and with releasing arms (37) which eliminate the lifting.
6. The apparatus according to any one of the Claims 1 to 5 characterised by that at least one of the cylinders (1) is equipped with an unit winding up the cutting unit (9), namely with a cutting gear wheel (15) and the stepping unit (3) is equipped with a unit eliminating the winding up of the cutting unit (9), namely a cylinder lifter (35).
7. The apparatus according to any one of the Claims 3 to 6 characterised by that the counter (7) is built up and fastened in the apparatus as an exchangeable unit.

Statement under Article 19

The difference between the original and the new claim 1 is that the new claim 1 includes in its main part the characteristic part of the original claim 1;

the new characteristic part of the new claim 1 includes the unchanged text of original claims 3-4.

1/5

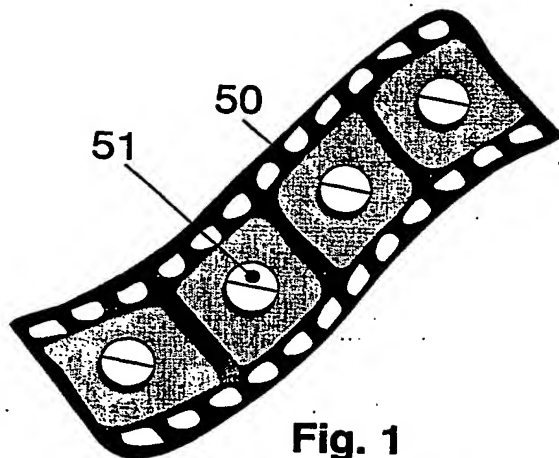


Fig. 1

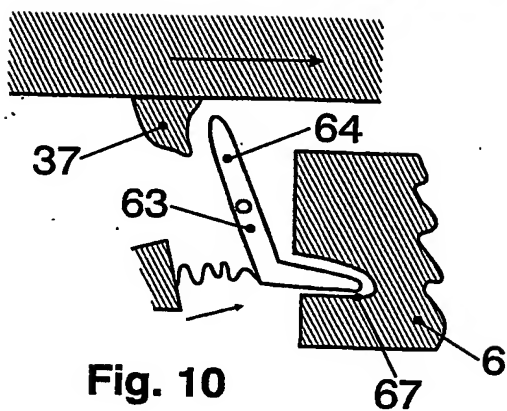


Fig. 10

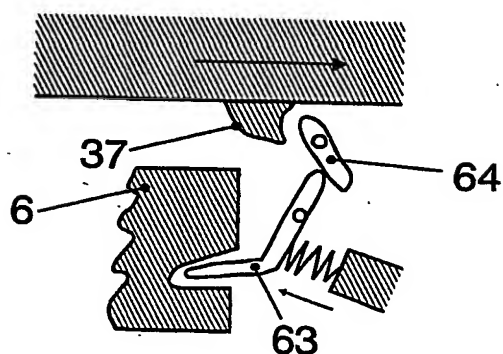


Fig. 11

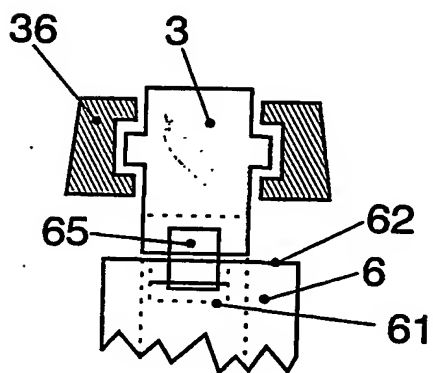


Fig. 12

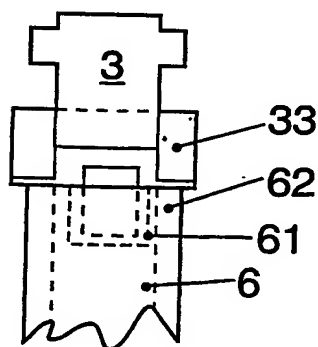


Fig. 13

2/5

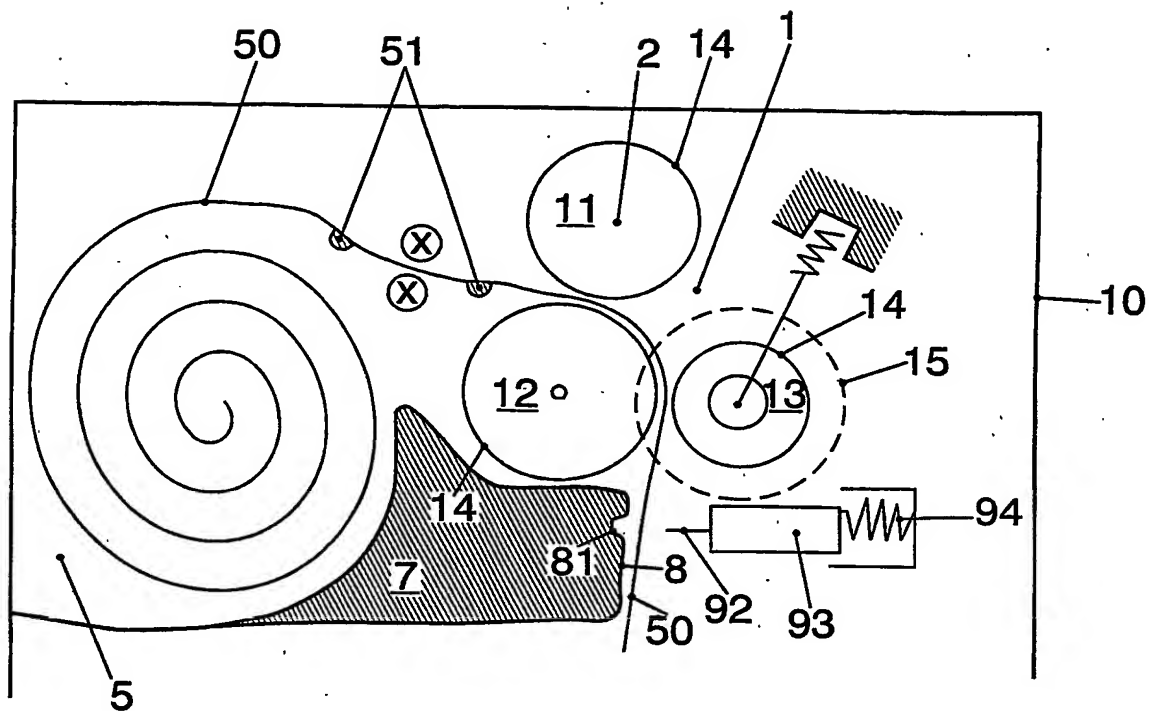


Fig. 6

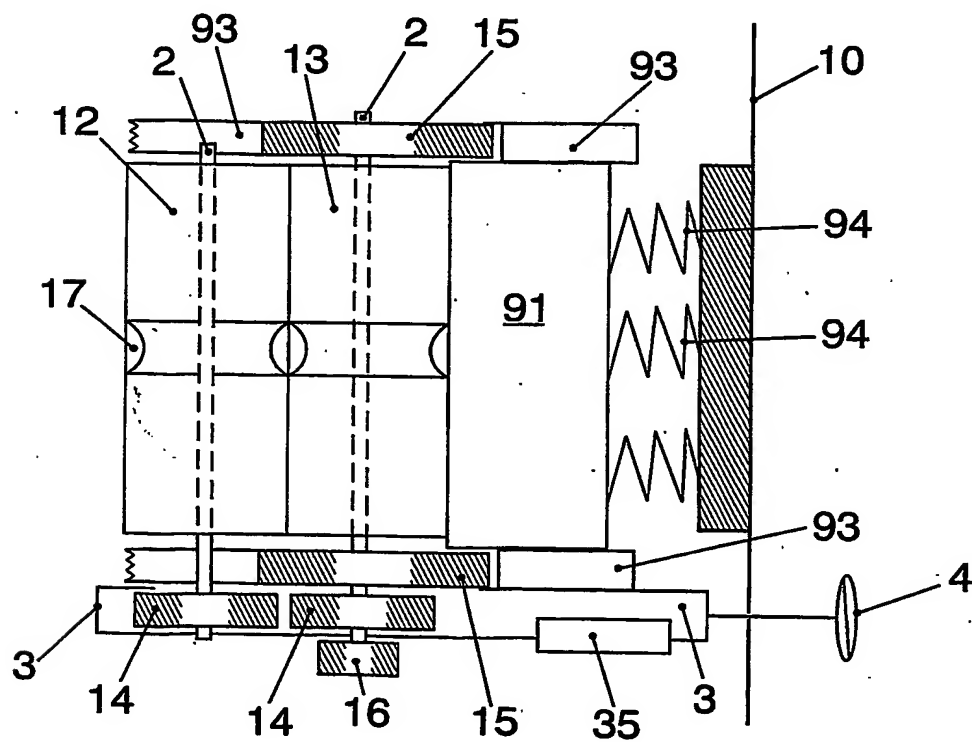


Fig. 7

3/5

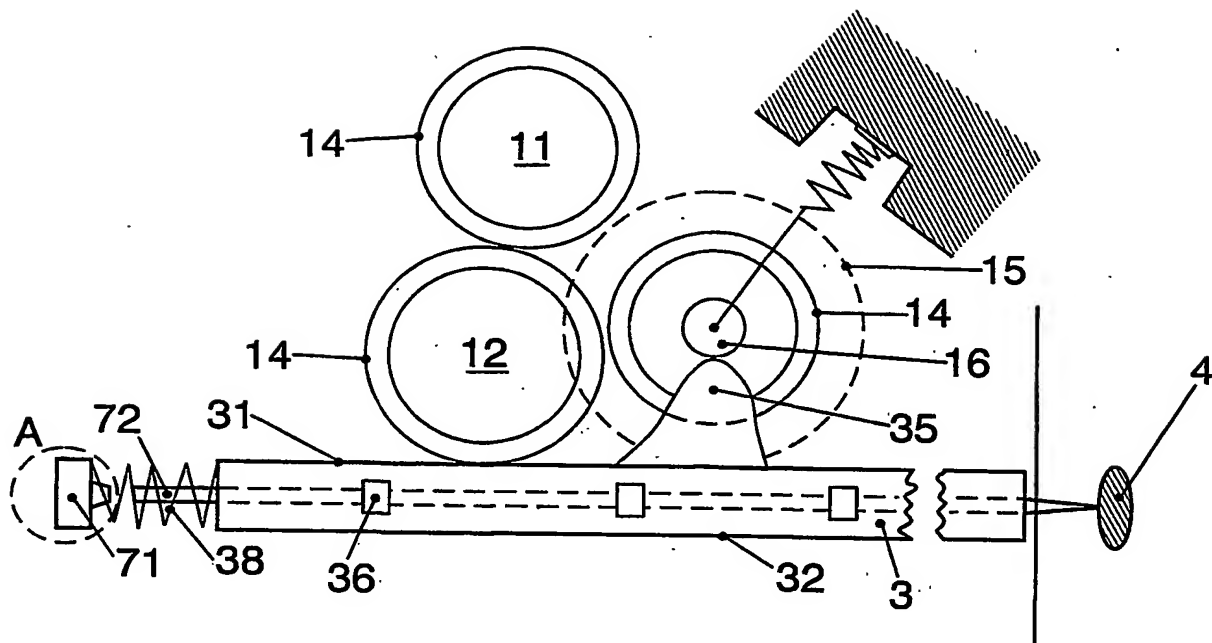


Fig. 8





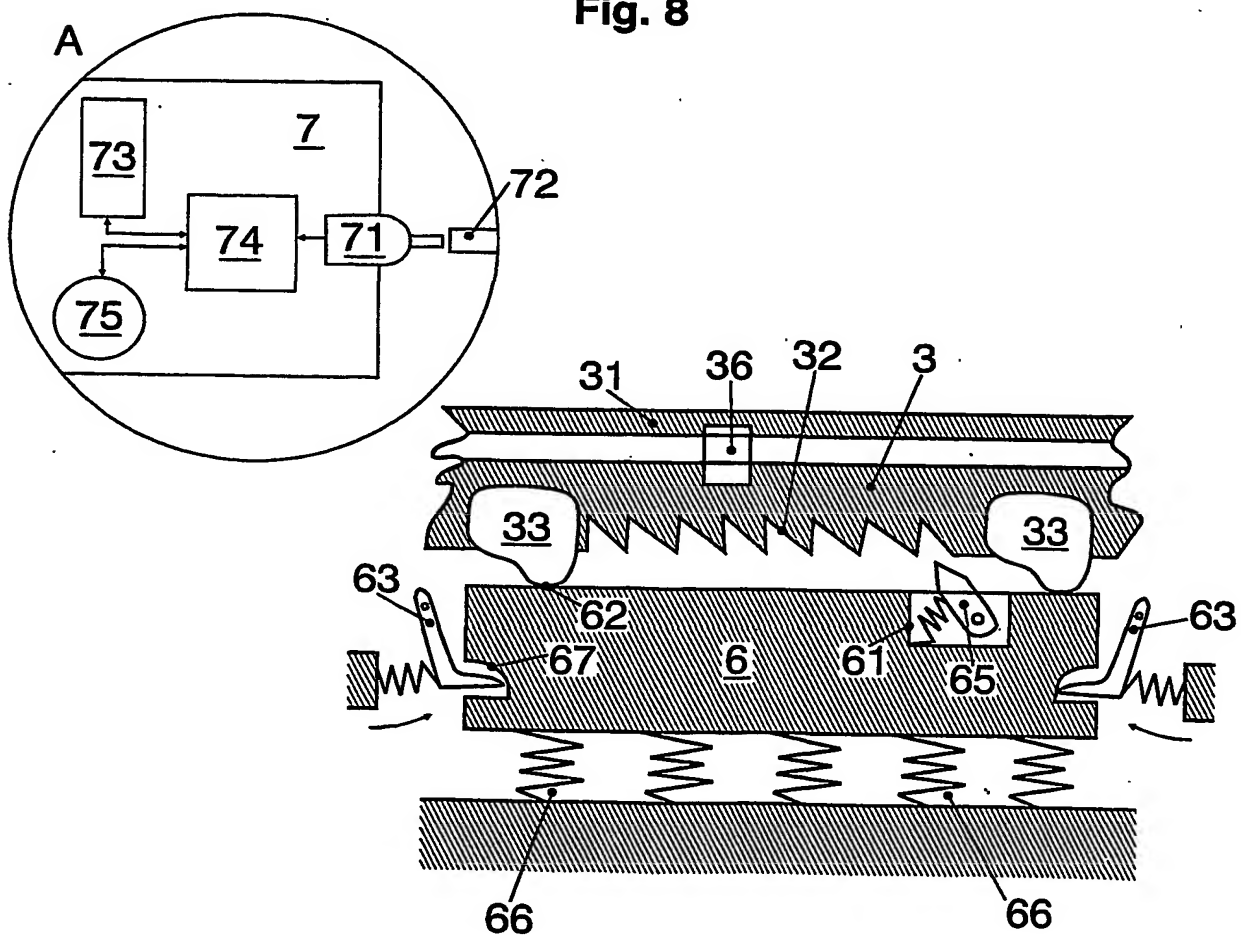


Fig. 9

4/5

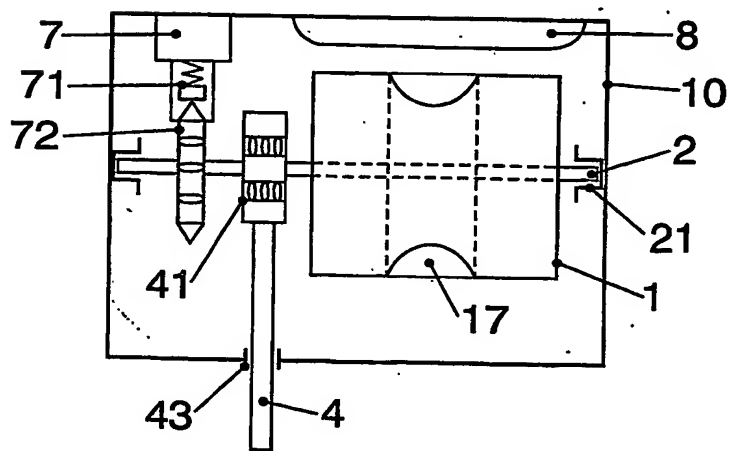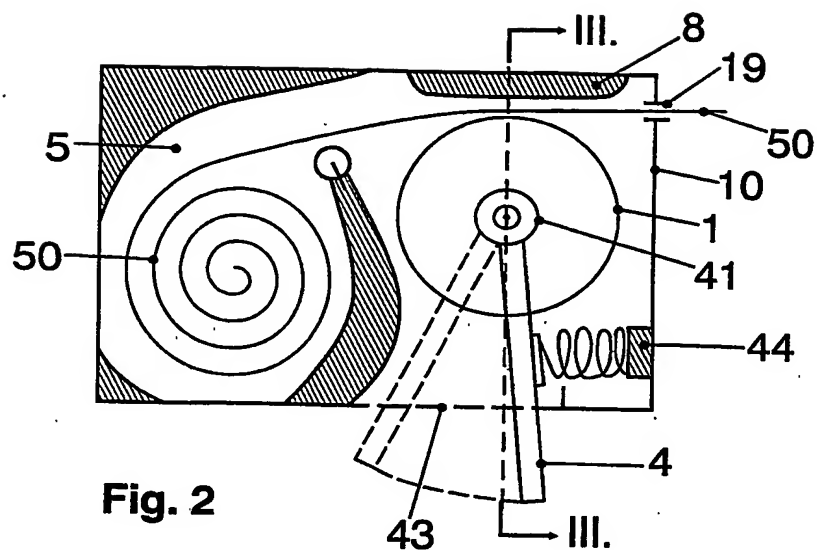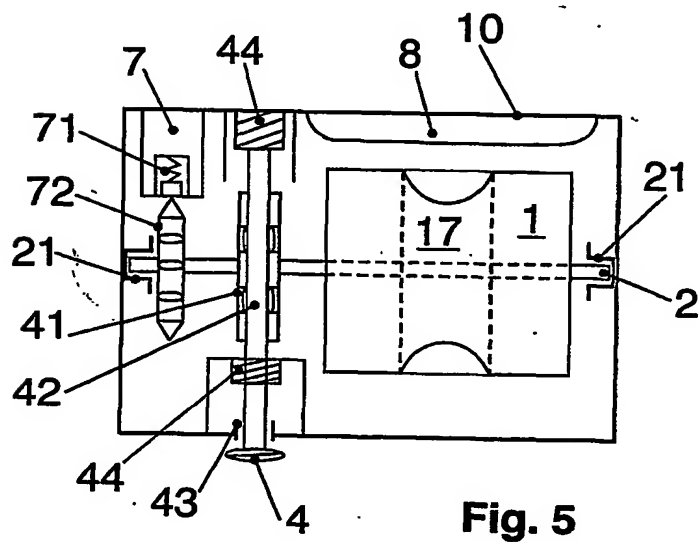

5/5

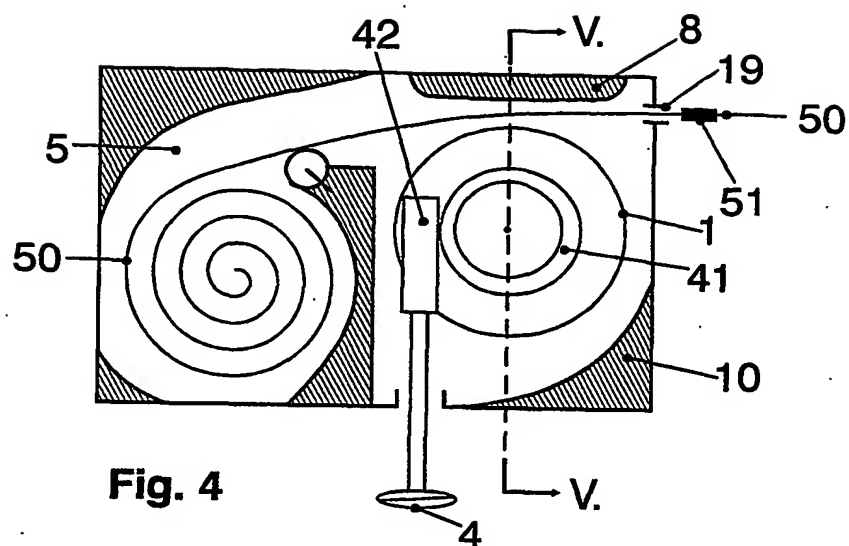

INTERNATIONAL SEARCH REPORT

International Application No

PCT/HU 01/00028

A. CLASSIFICATION OF SUBJECT MATTER

IPC 7 A61J7/00

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC 7 A61J B65D

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practical, search terms used)

EPO-Internal

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 4 274 550 A (FELDSTEIN GEORGE) 23 June 1981 (1981-06-23)	1,2
Y	the whole document	3,4,9
X	US 5 119 969 A (HABER TERRY M) 9 June 1992 (1992-06-09)	1,2
X	the whole document	
X	US 3 410 450 A (FORTENBERRY JERRY A) 12 November 1968 (1968-11-12)	1
A	column 4, line 72 -column 5, line 65; figures 9-14	3
X	US 4 733 797 A (HABER TERRY M) 29 March 1988 (1988-03-29)	1,2
	the whole document	
	--- -/--	



Further documents are listed in the continuation of box C.



Patent family members are listed in annex.

* Special categories of cited documents :

- *A* document defining the general state of the art which is not considered to be of particular relevance
- *E* earlier document but published on or after the international filing date
- *L* document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)
- *O* document referring to an oral disclosure, use, exhibition or other means
- *P* document published prior to the international filing date but later than the priority date claimed

- *T* later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
- *X* document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
- *Y* document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art.
- *G* document member of the same patent family

Date of the actual completion of the international search

18 June 2001

Date of mailing of the international search report

26/06/2001

Name and mailing address of the ISA

European Patent Office, P.B. 5818 Patentlaan 2
NL - 2280 HV Rijswijk
Tel (+31-70) 340-2040, Tx. 31 651 epo nl,
Fax (+31-70) 340-3016

Authorized officer

Godot, T

INTERNATIONAL SEARCH REPORT

International Application No.

PCT/HU 01/00028

C.(Continuation) DOCUMENTS CONSIDERED TO BE RELEVANT

Category *	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	US 3 985 264 A (SHAW JOSEPH DENMAN ET AL) 12 October 1976 (1976-10-12) column 5, line 51 - column 6, line 16; figures	3,4,9
A	US 3 732 544 A (OBLAND D) 8 May 1973 (1973-05-08) column 3, line 17 - line 19; figures	3,4,9
A	DE 198 35 940 A (JENAPHARM GMBH) 17 February 2000 (2000-02-17) column 4, line 22 - line 23; figure 4	3-5,9
A	WO 91 04726 A (VALDEMARSSON LARS) 18 April 1991 (1991-04-18) the whole document	3-5,9

INTERNATIONAL SEARCH REPORT

Information on patent family members

International Application No

PCT/HU 01/00028

Patent document cited in search report		Publication date	Patent family member(s)	Publication date
US 4274550	A	23-06-1981	NONE	
US 5119969	A	09-06-1992	US 5065655 A	19-11-1991
US 3410450	A	12-11-1968	NONE	
US 4733797	A	29-03-1988	NONE	
US 3985264	A	12-10-1976	NONE	
US 3732544	A	08-05-1973	NONE	
DE 19835940	A	17-02-2000	AU 6461599 A WO 0007904 A	28-02-2000 17-02-2000
WO 9104726	A	18-04-1991	SE 468540 B EP 0494952 A SE 8903297 A	08-02-1993 22-07-1992 07-04-1991